

Weightron Bilanciai Ltd,
Titan Works
Bridge Way off Broombank Road,
Chesterfield Trading Estate,
Chesterfield S41 9QJ, UK
Tel: 01246 260062
Fax: 01246 260844
www.weightron.com



Weightron Bilanciai Ltd,
Unit 4b, Block 4
Westpark, Chelston
Wellington TA21 9AD, UK
Tel: 01823 662355
Fax: 01823 662017
www.weightron.com



CALIBRATION CERTIFICATE

This Calibration Certificate is issued in accordance with the UKWF Code of Practice for the calibration of Non Automatic Weighing Machines. All weights used are traceable to NPL

Customer

WASTE LABO D
HINES PIT
WAREHOUSE
DN20 GAE
LOCATION

Machine Details

Cust ref	
Make	AVELY
Model	Z19 XUS
Ser No	162950158
Capacity	50000g /
e/d	20g / /
Working cap	

Test Weights

Set No.	Cert No.	Date Cal
PDG1-22	T211126	2/12/20

Cert Interval	12m
Next Cert	JAN 2022

Tolerance +/-	g
0 - 10000	20
10000 - 40000	40
40000 - 50000	60

Comments

MADE UP WEIGHTS USED

2

4

6

1


3

5

AS FOUND LINEARITY & HYSTERESIS

Load	Loading	Dev	Unloading	Dev
0	0	0	0	0
10000	10000	0	10000	0
20000	20000	0	20000	0
25540	25540	0	25540	0
24360	24360	0	24360	0
34360	34360	0	34360	0
44360	44360	0		

DEFINITIVE LINEARITY & HYSTERESIS

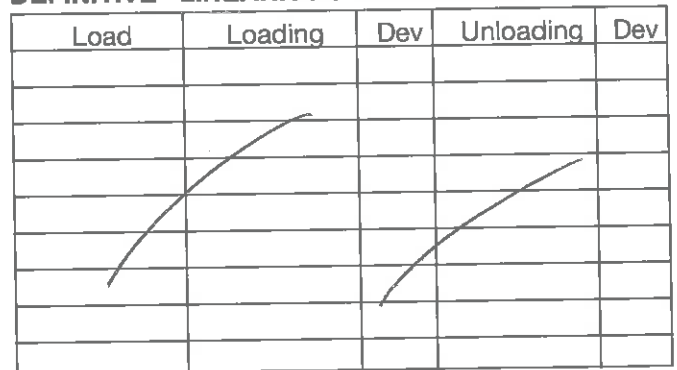

Repeatability

Load	Ind	Ind	Ind
44360	44360	44360	44360

Repeatability

Load	Ind	Ind	Ind

Eccentric Load

Reading	Dev	Reading	Dev
1	7540	2	7540
3	7540	4	7540
5	7540	6	7540
7		8	

Eccentric Load

Reading	Dev	Reading	Dev
1		2	
3		4	
5		6	
7		8	

Signature M. B. [Signature] Name M. B. [Signature] Date 29/1/2021
C1.3.88.1M